

Electroporator for *in vitro* cell permeabilization

Marko Puc, Karel Flisar, Stanislav Reberšek and Damijan Miklavčič

University of Ljubljana, Faculty of Electrical Engineering, Ljubljana, Slovenia

The use of high voltage electric pulse technology, electroporation, in cell biology, biotechnology and medicine has attracted an enormous interest. Electroporation is a transient phenomenon that increases the permeability of cell plasma membrane. In the state of high permeability, the plasma membrane allows small and large molecules to be introduced into the cytoplasm, although the cell plasma membrane represents a considerable barrier for them in its normal state. The effectiveness of electroporation depends on many parameters that can be divided into the parameters of the electric field and the parameters that define the state of cells and their surrounding, i.e. temperature, osmotic pressure, etc. In this article, we present a prototype electroporator **GT-1** for *in vitro* electroporabilization that we have developed. Our electroporator offers a vast flexibility of parameters and can generate high and low voltage pulses, of which the latter ones are used for electrophoretic transfer of charged molecules through permeabilized cell plasma membrane.

Key words: electroporation - instrumentation - methods; cell membrane permeabilization

Introduction

Viability of a cell depends on the integrity of its plasma membrane. The plasma membrane prevents the exchange of substances between intracellular and extracellular spaces. Exposing the cell to the electric field can increase the permeability of the cell plasma membrane. The increased permeability of the plasma membrane allows small and large molecules to be introduced into the cytoplasm. This phenomenon is transient and is

Received 6 July 2001

Accepted 3 August 2001

Correspondence to: dr. Damijan Miklavčič, University of Ljubljana, Faculty of Electrical Engineering, Tržaška 25, SI-1000 Ljubljana, Slovenia. Phone: +386 1 4768456; Fax: +386 1 4264658; E-mail: damijan@svarun.fe.uni-lj.si

termed electroporabilization and often also referred to as electroporation. The electroporation is widely used in different medical and biological applications i.e. electrochemotherapy, transdermal drug delivery and gene transfection. The effectiveness of all these applications depends on many parameters that can be divided into the parameters of the electric field and the parameters that define the state of cell and its surrounding, i.e. temperature, osmotic pressure, conductivity of cytoplasm and extracellular fluids etc. With respect to this, optimal parameters of electroporation have to be used to achieve best efficiency of the method.¹

For *in vitro* experiments, where most commonly used electrodes are parallel plates with a 2 mm inner distance, the threshold voltages typically range from 120 V to 300 V^{1,2}, with

the pulse durations from several microseconds to several milliseconds.^{1,3} Beside this, it is often necessary to deliver more than one pulse to increase efficiency of permeabilization. In that case, pulses must be delivered in a certain period requiring repetition frequencies from 1 Hz to several hundred Hz.

All these demands are fulfilled by special devices, often referred to as electroporators. Nowadays, there are a lot of commercially available electroporators that are designed for *in vitro* experiments. The problem of most of these electroporators is that the flexibility of the parameters of electric pulses is not sufficient, especially if we want to study the effects of different pulse parameters on the cell permeabilization, survival or average uptake of different molecules.

In this paper, we present the design of electroporator for *in vitro* cell plasma membrane permeabilization. The device is operated by an internal computer that allows the user to choose the parameters of electric field. The computer drives the pulse generator that is composed of a digital pulse generator generating the signal, high voltage amplifier amplifying the signal, and current

amplifier that provides the signal with sufficient energy to prevent the voltage amplitude from dropping during the pulse delivery. Beside this, the last version of the developed electroporator also includes a special unit that generates low voltage pulses usually used for the electrophoretic transfer of the charged molecules through the permeabilized cell plasma membrane.

System design

Figure 1 shows the basic system design of the electroporator. It consists of a computer, pulse generator, voltage amplifier, current amplifier and low voltage pulse generator. Besides this, the device comprises two high voltage power supplies and several low voltage devices that are necessary for normal operation but are not drawn on the figure.

The internal computer of the device is in the first place used for selecting pulse parameters. Therefore, the computer includes a user interface composed of a display and a keyboard. The second task of the computer is to control pulse generation after activation has

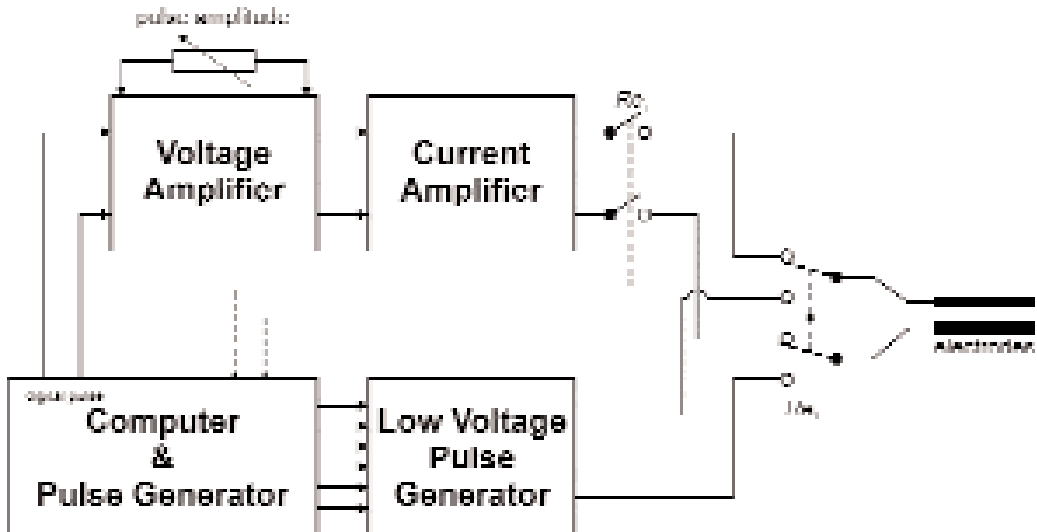


Figure 1. Block diagram of *in vitro* electroporator GT-1.

been triggered. All pulse parameters, except pulse amplitude, are then transferred to the pulse generator. This subunit generates digital signal that is then amplified in the voltage amplifier to the value that we set by external potentiometer. The amplified signal is then intensified by the energy from the current amplifier because we have to fulfill the energy requirement as defined by the load between electrodes.⁴ At this point, the generation of the high voltage signal that is used for permeabilization of cell plasma membrane is finished.

The low voltage pulse generator, which we have constructed just recently, is used for the electrophoretic transfer of charged molecules through permeabilized cell plasma membrane. The structure of this subunit, controlled by the internal computer, is similar to that of the DC power supply. This version allows to change the amplitude in 10 V steps in a range from 0 V to 50 V.

Performance and experimental results

The developed *in vitro* electroporator, which is still a prototype, has been used in our laboratory for more than two years. During that time, we found and repaired some deficiencies in design and we also made several other improvements that reflect on greater flexibility of the parameters. The current prototype **GT-1** allows the user to set high and low voltage pulses in a range that is given in Table 1. The pulse repetition frequency f is calculated by using the following equation:

$$f = \frac{1}{T \cdot (1 + D_R)}, \quad (1)$$

where T is pulse duration and D_R is value of the parameter Delay/Pulse ratio.

Furthermore, to demonstrate the performance of the device we designed an experiment where we measured voltage and current on the output (Fig. 2). In the experiment, we ex-

Table 1. Output parameters of the developed *in vitro* electroporator

Parameter	Value		
	Min.	Max.	Increment
HIGH VOLTAGE PULSES			
Pulse duration	5 μ s	5000 μ s	1 μ s & 50 μ s
Delay/Pulse ratio*	3	65535	1
Pulse amplitude	25V	500V	linear
Number of pulses	1	128	1
Pulse current		30A	
LOW VOLTAGE PULSES			
Pulse duration	5ms	9999ms	1ms
Delay duration	0ms	9999ms	1ms
Pulse amplitude	0V	50V	10V
Number of pulses	1	1000	1
Pulse current		1A	

* - parameter defines pulse repetition frequency that is calculated by the equation (1).

posed 50 μ l of pure SMEM, which was placed between 2mm plate electrodes, to five consecutive 100 μ s pulses of 500 V at a repetition frequency of 2.5 kHz ($D_R = 3$).

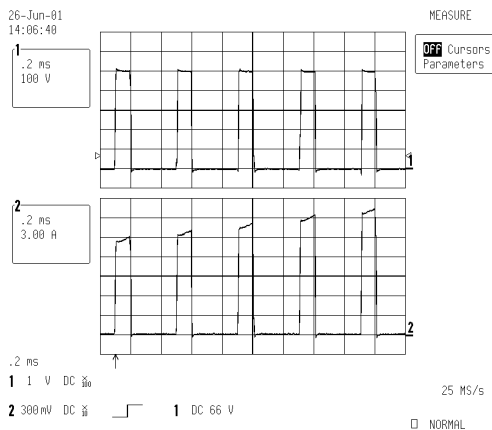


Figure 2. Performance of electroporator loaded with 50 μ l drop of SMEM that was placed between 2 mm plate electrodes. Electroporator was programmed to generate five consecutive 100 μ s pulses of 500 V and repetition frequency of 2.5 kHz ($D_R = 3$). Top trace (signal 1) presents voltage and bottom trace (signal 2) presents current flowing through the system. The measurements were performed using LeCroy LT9310C digital oscilloscope, a LeCroy AP015 current probe, and a Tektronix P5100 1:100 voltage probe. The voltage was 500 V, while current increased from 14 A to 19 A.

It is evident from the Figure 2 that the instrument was able to deliver all the pulses without any distortion. Even more, it could easily increase the current between two consecutive pulses that is usually necessary due to the polarization of the sample between the electrodes.

To compare the performance of the prototype **GT-1** with that of Jouan GHT 1287B, we evaluated cell permeabilization, using a bleomycin method⁵, with both devices. The results of experiments that are shown on Figure 3 are comparable. T-test showed no statistically significant difference between both experiments.

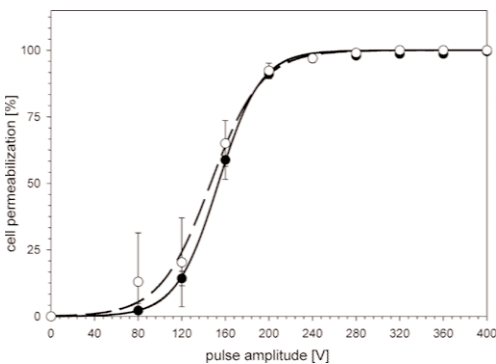


Figure 3. Comparison of cell permeabilization as a function of pulse amplitude obtained with electropulsator Jouan GHT 1287B (●), and *in vitro* electroporator GT-1 (○).

Besides the performance experiments that we carried out, our colleagues already published the results of the experiments using the developed electroporator.^{6,7} The two experiments were performed to study the influence of the parameters of electroporation (medium conductivity⁶ and pulse repetition frequency⁷) on the cell permeabilization, survival and average uptake.

Conclusions

The comparison of the developed prototype

Radiol Oncol 2001; 35(3): 203-7.

GT-1 with the commercially available device Jouan showed that **GT-1** fulfils all demands of the *in vitro* investigations. Furthermore, it offers a vast flexibility of the parameters and has the ability to generate high and low voltage pulses, where low voltage pulses can be used for the electrophoretic transfer of charged molecules through permeabilized cell plasma membrane.

Acknowledgment

Our research was supported through various grants by the Ministry of Education, Science and Sports of the Republic of Slovenia and in part by IGEA s.r.l. Italy. Authors wish to thank to Maša Kandušar D.Sc., Tadej Kotnik D.Sc, and Gorazd Pucihar B.S. who performed many experiments with the developed prototypes and provided us with a wealth of feedback information about operation of devices.

References

1. Mir LM. Therapeutic perspectives of *in vivo* cell electroporation. *Bioelectrochemistry* 2000; **53**: 1-10.
2. Čemažar M, Jarm T, Miklavčič D, Maček-Lebar A, Ihan A, Kopitar NA, Serša G. Effect of electric-field intensity on electroporation and electrosensitivity of various tumor-cell lines *in vitro*. *Electro Magnetobiol* 1998; **17**: 261-70.
3. Tsong TY. Electroporation of cell membranes. *Biophys J* 1991; **60**: 297-306.
4. Puc M, Reberšek S, Miklavčič D. Requirements for a clinical electrochemotherapy device - electroporator. *Radiol Oncol* 1997; **31**: 368-73.
5. Kotnik T, Maček-Lebar A, Miklavčič D, Mir LM. Evaluation of cell membrane electroporation by means of a nonpermeant cytotoxic agent. *Biotechniques* 2000; **28**: 921-6.
6. Pucihar G, Mir LM, Miklavčič D. The effect of pulse repetition frequency on Lucifer Yellow up-

take by means of cell electroporabilization in vitro. In Magjarević R, Tonković S, Bilas V, Lacković I, editors. *IFMBE Proceedings*. Pula: Biotisak; 2001. p. 834-6.

7. Pucihar G, Kotnik T, Kandušer M, Miklavčič D. The influence of medium conductivity on electroporabilization and survival of cells *in vitro*. *Bioelectrochemistry* 2001; (accepted - in print).